

Mi180

pH/ORP/EC/TDS/NaCl/Temperature Laboratory Bench Meter

Mi180 measures 6 different parameters: pH, ORP, EC, TDS (Total Dissolved Solids), percentage of NaCl and temperature in a variety of ranges.

pH calibration can be performed in 3 points selectable between 7 memorized buffers, to provide a very accurate calibration curve even when testing different samples, where very wide differences in pH can be found.

The auto-ranging feature for EC and TDS measurements automatically sets the resolution suitable to the tested sample. All measurements can be temperature compensated at 20 or 25°C and the compensation coefficient is selectable by the user.

The automatic temperature compensation can also be disabled for measuring the actual conductivity value. The stability indicator on the LCD ensures accuracy. Conductivity readings are performed with the 4-ring probe supplied with the meter.

The GLP feature allows users to store and recall data on system status.



PC compatible through an RS232 port or USB.

Years warranty
3

LOG

MEM

RS232

USB

ATC

GLP

Points
2

Dual Display

MULTI

Software CD

Self diagnostics

CE

| Specifications | | Mi180 |
|----------------------------|---|---|
| Range | pH mV EC TDS NaCl Temp | -2.00 to 16.00 pH; -2.000 to 16.000 pH ±699.9 mV; ±2000 mV 0.00 to 29.99 µS/cm; 30.0 to 299.9 µS/cm; 300 to 2999 µS/cm; 3.00 to 29.99 mS/cm; 30.0 to 200.0 mS/cm; up to 500.0 mS/cm (uncompensated EC*) 0.0 to 14.99 mg/L (ppm); 15.0 to 149.9 mg/L (ppm); 150 to 1499 mg/L (ppm); 1.50 to 14.99 g/L (ppt); 15.0 to 100.0 g/L (ppt); up to 400.0 g/L actual TDS (with 0.80 factor) 0.0 to 400.0% -20.0 to 120.0°C / -4.0 to 248.0°F |
| Resolution | pH mV EC TDS NaCl Temp | 0.01 pH; 0.001 pH 0.1 mV; 1 mV 0.01 µS/cm; 0.1 µS/cm; 1 µS/cm; 0.01 mS/cm; 0.1 mS/cm; 0.01 mg/L; 0.1 mg/L; 1.0 mg/L; 0.01 g/L; 0.1 g/L 0.1% 0.1°C / 0.1°F |
| Accuracy | pH mV EC TDS NaCl Temp | ±0.01 pH; ±0.002 pH ±0.2 mV; ±1 mV ±1% of reading ±(0.05 µS/cm or 1 digit) ±1% of reading ±(0.03 ppm or 1 digit) ±1% reading ±0.4°C / ±0.8°F |
| Rel mV offset | | ±2000 mV |
| Calibration | pH EC NaCl Temp | 1, 2 or 3 points calibration, with 7 memorized buffers (pH 1.68, 4.01, 6.86, 7.01, 9.18, 10.01 and 12.45) 1 point slope calibration with 6 memorized solutions: (84 µS/cm, 1413 µS/cm, 5.00 mS/cm, 12.88 µS/cm, 80.0 µS/cm, 111.8 mS/cm) 1 point, with MA9066 solution 2 point, at 0 and 50°C / 32 and 122°F |
| Temperature Compensation | | automatic or manual, from -20.0 to 120.0°C / -4.0 to 248.0°F |
| Temperature Coefficient | | selectable from 0.00 to 6.00%/°C (EC and TDS only) |
| pH Electrodes & Temp Probe | | MA917B/1 & MA831R (included) |
| EC/TDS/NaCl/Temp Probe | | MA814DB/1 (included) |
| TDS Factor | | 0.40 to 0.80 (default value is 0.50) |
| Logging | | up to 50 records, LOG on demand or auto-logging |
| GLP | | last pH, EC, NaCl calibration data |
| PC Interface | | RS232 / USB Opto-isolated |
| Environment | | 0 to 50°C / 32 and 122°F; max RH 95% |
| Input Impedance | | 10 ¹² Ohm |
| Power supply | | 12 VDC power adapter (included) |
| Dimensions | | 230 x 160 x 95 mm |
| Weight | | 0.9 kg |

(*) Uncompensated conductivity (or TDS) is the conductivity (or TDS) value without temperature compensation.

Ordering Information

Mi180 is supplied complete with

- MA917B/1 pH Electrode
- MA814DB/1 EC/TDS/NaCl/Temperature probe
- MA831R Temperature Probe

- MA9315 Electrode Holder
- M10004 pH 4.01 Sachet Buffer solution
- M10007 pH 7.01 Sachet Buffer solution
- M10010 pH 10.01 Sachet Buffer solution
- M10030 12880 µS/cm calibration solution
- M10031 1413 µS/cm calibration solution

Accessories




- MA9004 pH 4.01 buffer, 230 mL bottle
- MA9007 pH 7.01 buffer, 230 mL bottle
- MA9010 pH 10.01 buffer, 230 mL bottle
- MA9015 Electrode storage solution, 230 mL bottle
- MA9016 Electrode cleaning solution, 230 mL bottle
- MA9112 pH 12.45 buffer solution, 230 mL bottle
- MA9060 12880 µS/cm calibration solution, 230 mL bottle
- MA9061 1413 µS/cm calibration solution, 230 mL bottle
- MA9063 84 µS/cm calibration solution, 230 mL bottle
- MA9065 111.8 mS/cm calibration solution, 230 mL bottle
- MA9066 100% NaCl calibration solution, 230 mL bottle
- MA9069 5000 µS/cm solution, 230 mL bottle
- MA9310 12 VDC Adapter, 220 V
- MA9311 12 VDC Adapter, 110 V
- MA9315 Electrode Holder
- MA917B/1 Double junction refillable pH electrode
- MA814DB/1 EC/TDS/NaCl/Temperature probe with DIN connector and 1 m cable
- MA921B/1 Platinum ORP electrode with 1 m cable (will be replaced by SE310)
- SE300 Platinum ORP electrode with 1 m cable
- MA831R Temperature probe
- MA9350 RS232 connection cable with 2 meters cable

- M10016 Sachet Electrode Cleaning solution
- Mi5200 Application Software
- MA9350 RS232 connection cable with 2 meters cable

Click to buy: www.easeongear.com

Mi805/Mi806

Portable pH/EC/TDS/Temperature Meters



Measures 4 parameters with 1 single probe. **Mi805** and **Mi806** offer you a combination of pH, Conductivity, total dissolved solids and temperature measurements.

You can select from a range of calibration buffers and also the temperature scale (°C or °F) can be selected.



The multi-parameter probe MA851D/1, includes pH/EC/TDS and temperature, all in one rugged handle.

Other features include different TDS factors from 0.45 to 1.00, and a range of temperature coefficients (B) from 0.0 to 2.4% for greater consistency and reproducibility. The Stability Indicator prompts the user when the reading stabilizes.

The Auto-Hold Function automatically freezes reading for later viewing. Large and Easy-to-Read display provides simultaneous readings of pH and Temperature or EC/TDS and temperature.



Specifications

| | |  |  |
|--------------------------|-------------------------|---|---|
| | | Mi805 | Mi806 |
| Range | pH EC TDS Temp | 0.00 to 14.00 pH 0 to 3999 µS/cm 0 to 1999 ppm 0.0 to 60.0°C / 32.0 to 140.0°F | 0.00 to 14.00 pH 0.00 to 20.00 mS/cm 0.00 to 10.00 ppt 0.0 to 60.0°C / 32.0 to 140.0°F |
| Resolution | pH EC TDS Temp | 0.01 pH 1 µS/cm 1 ppm 0.1°C / 0.1°F | 0.01 pH 0.1 mS/cm 0.01 ppt 0.1°C / 0.1°F |
| Accuracy (@25°C) | pH EC/TDS Temp | ±0.01 pH ±2% Full Scale ±0.5°C / ±1°F | ±0.01 pH ±2% Full Scale ±0.5°C / ±1°F |
| Typical EMC Deviation | pH EC/TDS Temp | ±0.02 pH ±2% Full Scale ±0.5°C / ±1°F | ±0.02 pH ±2% Full Scale ±0.5°C / ±1°F |
| Temperature Compensation | | automatic from 0 to 60°C; with B adj. from 0.0 to 2.4%/°C | automatic from 0 to 60°C; with B adj. from 0.0 to 2.4%/°C |
| pH Calibration | | automatic, 1 or 2-point with automatic buffer recognition | automatic, 1 or 2-point with automatic buffer recognition |
| EC Calibration | | automatic, 1 point | automatic, 1 point |
| EC/TDS Conversion Factor | | adj. from 0.45 to 1.00 | adj. from 0.45 to 1.00 |
| Probe | | MA851D/1 amplified pH/EC/TDS/Temperature probe with DIN connector and 1 m cable (included) | MA851D/1 amplified pH/EC/TDS/Temperature probe with DIN connector and 1 m cable (included) |
| Environment | | 0 to 50°C / 32 to 122°F; max. RH 100% | 0 to 50°C / 32 to 122°F; max. RH 100% |
| Battery Type | | 1 x 9V alkaline (included) | 1 x 9V alkaline (included) |
| Battery Life | | approx. 300 hours | approx. 300 hours |
| Auto-off | | after 8 minutes of non-use | after 8 minutes of non-use |
| Dimensions | | 200 x 85 x 50 mm | 200 x 85 x 50 mm |
| Weight | | 260 g (with battery) | 260 g (with battery) |

Accessories



- MA851D/1** Amplified pH/EC/TDS/Temperature probe with DIN connector and 1 m cable
- MA9004** pH 4.01 buffer solution, 230 mL bottle
- MA9006** pH 6.86 buffer solution, 230 mL bottle
- MA9007** pH 7.01 buffer solution, 230 mL bottle
- MA9009** pH 9.18 buffer solution, 230 mL bottle
- MA9010** pH 10.01 buffer solution, 230 mL bottle
- MA9015** Probe storage solution, 230 mL
- MA9016** General cleaning solution, 230 mL
- MA9060** 12880 µS/cm solution, 230 mL
- MA9061** 1413 µS/cm solution, 230 mL
- M10000B** Rinse solution, 20 mL (25 pcs.)

Ordering Information

Mi805 is supplied complete with MA851D/1 pH/EC/TDS/Temp amplified probe with 1 meter cable, 2x20 mL pH 4.01 and pH 7.01 sachet of calibration solution, 2x20 mL 1413 µS/cm sachet of calibration solutions, 2x20 mL sachet of electrode cleaning solutions, rugged carrying case, 9V battery and instructions.

Mi806 is supplied complete with MA851D/1 pH/EC/TDS/Temp amplified probe with 1 meter cable, 2x20 mL pH 4.01 and pH 7.01 sachet of calibration solution, 2x20 mL 12880 µS/cm sachet of calibration solutions, 2x20 mL sachet of electrode cleaning solutions, rugged carrying case, 9V battery and instructions.

MW801/MW802

Entry level, inexpensive pH/EC/TDS Portable Meters for fast and reliable results

MW801 and **MW802** are compact Portable Meters with Faster Micro Processor. These meters allow you to measure pH, EC (conductivity) and TDS with just one instrument and one single probe!



These easier and faster to calibrate portable meters have a smaller, ergonomic and lighter case design. Other features include 100% larger and easier to read LCD Display and long battery life.

Both meters calibrate manually in pH, Conductivity and TDS.

Each meter is supplied with the MA850 interchangeable probe with 1 meter cable to measure pH, Conductivity and TDS. The pH electrode utilizes a fiber junction to reduce contamination when measuring fertilizer solutions.

- The **MW801** with a Conductivity range that goes up to 1990 $\mu\text{S/cm}$ and TDS range that goes up to 1990 ppm is an ideal tool for drinking water measurements.
- The **MW802**, with a conductivity range that goes up to 6.00 mS/cm and the TDS up to 4000 ppm is ideal for testing in crop production.



| Specifications | | MW801 | MW802 |
|-----------------------------|-----------------|---|---|
| | |  |  |
| Range | pH EC TDS | 0.0 to 14.0 pH 0 to 1990 $\mu\text{S/cm}$ 0 to 1990 ppm | 0.00 to 14.00 pH 0.00 to 6.00 mS/cm 0 to 4000 ppm |
| Resolution | pH EC TDS | 0.1 pH 10 $\mu\text{S/cm}$ 10 ppm | 0.10 pH 0.10 mS/cm 10 ppm |
| Accuracy (@20°C) | pH EC/TDS | ± 0.2 pH $\pm 2\%$ Full Scale | ± 0.20 pH $\pm 2\%$ Full Scale |
| Calibration Solutions | | M10007 (pH 7.01) M10032 (1382 ppm) M10031 (1413 $\mu\text{S/cm}$) | M10007 (pH 7.01) M10442 (1500 ppm) M10031 (1413 $\mu\text{S/cm}$) |
| Conversion Factor | | 0.5 | 0.68 |
| Calibration | | manual, at 1 point | manual, at 1 point |
| Temperature Compensation | | automatic, from 0 to 50°C | automatic, from 0 to 50°C |
| Probe | | SE600 combination pH/EC/TDS probe | SE600 combination pH/EC/TDS probe |
| Environment | | 0 to 50°C / 32 to 122°F; max RH 95% | 0 to 50°C / 32 to 122°F; max RH 95% |
| Battery Type / Battery Life | | 1 x 9 V alkaline / 150 hours of use | 1 x 9 V alkaline / 150 hours of use |
| Auto-off | | after 8 minutes of non-use | after 8 minutes of non-use |
| Dimensions | | 185 x 82 x 45 mm | 185 x 82 x 45 mm |
| Weight | | 165 g (with battery) | 165 g (with battery) |

Large and Easy-to-read Display

MW801 and MW802 offer highly stable and accurate readings with large LCD display.



Combined interchangeable pH, Conductivity and TDS Probe

The pH electrode utilizes a fiber junction to reduce contamination when measuring fertilizer solutions.



Accessories

- M10004B** pH 4.01 buffer solution, 20 mL sachet (25 pcs)
- M10007B** pH 7.01 buffer solution, 20 mL sachet (25 pcs)
- M10010B** pH 10.01 buffer solution, 20 mL sachet (25 pcs)
- M10031B** 1413 $\mu\text{S/cm}$ calibration solution, 20 mL sachet (25 pcs)

- M10032B** 1382 ppm calibration solution, 20 mL sachet (25 pcs)
- M10442B** 1500 ppm calibration solution, 20 mL sachet (25 pcs)
- MA9015** Electrode storage solution, 230 mL bottle
- SE600** pH/EC/TDS spare probe with 1 m cable



Ordering Information

MW801 is supplied complete with SE600 combination pH/EC/TDS probe, 20 mL sachet pH 7.01 buffer solution, 20 mL 1413 $\mu\text{S/cm}$ sachet of calibration solution, 20 mL 1382 ppm sachet of calibration solution, 9V battery and instructions.

MW802 is supplied complete with SE600 combination pH/EC/TDS probe, 20 mL sachet pH 7.01 buffer solution, 20 mL 1413 $\mu\text{S/cm}$ sachet of calibration solution, 20 mL 1500 ppm sachet of calibration solution, 9V battery and instructions.

Click to buy: www.easeongear.com

MW700

Entry level, inexpensive LUX Portable Meters for fast and reliable results

MW700 is a portable Lux meter designed to perform light measurements. MW700 with Faster Micro Processor, has a smaller, ergonomic and lighter case design. Other features include 100% larger and easier to read LCD Display and long battery life.

These handy and ergonomically designed portable meters are ideal for anyone working on a low budget and still requires fast and reliable measurements. These portable meters are suitable for a wide range of applications, such as Educational, Agriculture and Horticulture, as well as water and environmental analysis. Both models are supplied with a light sensor connected to the meter that measures from 0 to 50000 Lux. Average indoor lighting ranges from 100 to 1000 Lux and average outdoor sun lights about 50000 Lux. Lux is a unit that indicates the density of light that falls on a surface.

The light is necessary for the development of the plants. In fact, it is necessary a sufficient contribution of light in order to favor the photosynthesis and the closing of the plants. The supplement of light by means of lamps electrical workers is the method simpler and economic in order to bring the necessary light to the plants.

The human eye is sensitive only to blue, green, and red light, so in calculating the Lux falling on an object, only the light that the human eye sees is counted. When only infrared light falls on an object, the Lux is counted as zero since our eyes see nothing. Mathematically, a spectral weighting function becomes convolved with the actual illumination spectrum to calculate Lux exactly.

This is the formal definition of Lux and it makes Lux an unusual unit of measure.

Still, Lux can be thought of as a way of measuring light in terms of what our eyes perceive. The metric unit of measure for luminance of a surface. One Lux is equal to one Lumen per square meter. One Lux equals 0.0929 footcandles.

Light Sensor

MW700 are provided with a light sensor connected to the meter through a coaxial cable.



Range keys

Press one of the three "Range keys" to select the proper scale according to the intensity of the light.

| Specifications | MW700 |
|--------------------|--|
| Range | 0.000 to 1999 Lux 2000 to 19999 Lux 20000 to 50000 Lux |
| Range setting | manual through key buttons |
| Resolution | 1 Lux 10 Lux 100 Lux |
| Accuracy | ±6% of reading ±1 digit |
| Peak Wave Length | 560 nm |
| Sensor Type | silicon photodiode |
| Sensor Sensitivity | 100 scotopic Lux |
| Sensor Stability | ±2% change per year (in the first two years) |
| Environment | 0 to 50°C / 32 to 122°F; max RH 95% |
| Battery Type | 1 x 9V (IEC 6LR61) alkaline |
| Battery Life | approximately 150 hours of continuous use |
| Auto-off | after about 5 minutes of non-use |
| Weight | approximately 270 g (meter with sensor) |

Ordering Information

MW700 is supplied complete with 9V battery and instructions.



Mi411

Free & Total Chlorine and pH Photometer

This latest laboratory grade Microprocessor photometer has an excellent repeatability and is ideal for field measurements.

Chlorine is the most commonly used water disinfectant. Applications vary from treatment of drinking water and waste-water to pool and spa sanitization and food processing to sterilization.

Martini Instruments has developed the **Mi411**, a portable microprocessor based instrument to measure three critical parameters to ensure good water quality: pH, free chlorine and total chlorine.

This instrument provides greater resolution, better accuracy and immediate results.

Mi411 is supplied in a hard carrying case including 2 cuvetts, reagents for 100 tests, wiping tissue and instruction manual.

3 in 1 Combination Photometer!



| Specifications | | Mi411 Free & Total Chlorine and pH |
|----------------|---------------------------------------|---|
| Range | Free Chlorine Total Chlorine pH | 0.00 to 5.00 mg/L Cl ₂ 0.00 to 5.00 mg/L Cl ₂ 6.5 to 8.0 pH |
| Resolution | Free Chlorine Total Chlorine pH | 0.01 mg/L (0.00 to 3.50 mg/L); 0.10 mg/L (above 3.50 mg/L) 0.01 mg/L (0.00 to 3.50 mg/L); 0.10 mg/L (above 3.50 mg/L) 0.1 pH |
| Accuracy | Free Chlorine Total Chlorine pH | ±0.04 mg/L @1.50 mg/L ±0.04 mg/L @1.50 mg/L ±0.1 pH @7.2 pH |
| Method | Free Chlorine Total Chlorine pH | adaptation of the USEPA method 330.5 and Standard Method 4500-Cl G adaptation of the USEPA method 330.5 and Standard Method 4500-Cl G adaptation of the phenol red method |
| Light Source | | tungsten lamp |
| Light Detector | | silicon photocell and 525 nm narrow band interference filter |
| Environment | | 0 to 50°C / 32 to 122°F; max RH 100% |
| Battery Type | | 1 x 9V |
| Auto-off | | after 10 minutes of non-use |
| Dimensions | | 192 x 104 x 52 mm |
| Weight | | 380 g |



Hard Carrying Case

Mi411 comes complete in hard carrying case, making it ideal for field measurements.

Accessories

Mi504-100 Free & Total Chlorine reagent set (100 tests)

Mi509-100 pH reagent (100 tests)

Mi511-100 Free & Total Chlorine and pH reagent set (100 tests)

Mi524-100 Total Chlorine powder reagents (100 tests)

Mi526-100 Free Chlorine powder reagents (100 tests)

Mi0001

Mi0002

Mi0003

Mi0005

Glass cuvetts (2 pcs)

Caps for cuvetts (2 pcs)

Stoppers for cuvetts (2 pcs)

9V battery (1 pc)

Ordering Information

Mi411 is supplied complete with 2 cuvetts, Mi511-100 liquid reagents for 100 tests, hard carrying case, wiping tissue, 9V battery and instructions.

Click to buy: www.easeongear.com

Mi405/Mi407/Mi408/Mi412 Ammonia, Iron & Phosphate Photometers

These user-friendly Colorimeters will give you direct readings in mg/L.





Ammonia detection in water treatment systems is particularly important for aquarium owners and fish farm operators. Ammonia is highly soluble in water and extremely toxic to fish. Fish farm owners must monitor and maintain careful control of ammonia levels to ensure optimum water conditions for their stock. Milwaukee offers 2 instruments for low and medium concentrations: **Mi405** with a range of 0.00 to 9.99 mg/L and **Mi407** from 0.00 to 3.00 mg/L

Iron is naturally present in water supplies and its presence in both potable and industrial applications is regarded as objectionable. Milwaukee offers **Mi408** Iron meter with a range of 0.00 to 5.00 mg/L.

Phosphates are present in natural waters and at concentrations typically found, do not pose any specific health threats to humans. However, excessive contamination of water courses from agricultural fertilizer run off or wastewater/effluent discharge can promote excessive algae or plant growth. Milwaukee offers **Mi412** with range 0.00 to 2.50 mg/L.



Specifications

| | |  Mi405 Ammonia MR |  Mi407 Ammonia LR |  Mi408 Iron HR |  Mi412 Phosphate LR |
|----------------|------------------------------|--|--|--|--|
| Range | Ammonia Iron Phosphate | 0.00 to 9.99 mg/L (NH ₃ -N) | 0.00 to 3.00 mg/L (NH ₃ -N) | 0.00 to 5.00 mg/L Fe | 0.00 to 2.50 mg/L PO ₄ |
| Resolution | Ammonia Iron Phosphate | 0.01 mg/L | 0.01 mg/L | 0.01 mg/L | 0.01 mg/L |
| Accuracy | Ammonia Iron Phosphate | ±0.10 mg/L @5.00 mg/L | ±0.04 mg/L @1.50 mg/L | ±0.03 mg/L @1.50 mg/L | ±0.04 mg/L @1.00 mg/L |
| Method | | adaptation of Nessler method | adaptation of Nessler method | adaptation of the USEPA method 315 B and Standard method 3500 - Fe B | adaptation of Ascorbic Acid method |
| Light Source | | Blue LED 466 nm | Blue LED 466 nm | tungsten lamp | tungsten lamp |
| Light Detector | | silicon photocell and 466 nm narrow band interference filter | silicon photocell and 466 nm narrow band interference filter | silicon photocell and 525 nm narrow band interference filter | silicon photocell and 610 nm narrow band interference filter |
| Environment | | 0 to 50°C / 32 to 122°F; max RH 100% | 0 to 50°C / 32 to 122°F; max RH 100% | 0 to 50°C / 32 to 122°F; max RH 100% | 0 to 50°C / 32 to 122°F; max RH 100% |
| Battery Type | | 1 x 9 volt | 1 x 9 volt | 1 x 9 volt | 1 x 9 volt |
| Auto-off | | after 10 minutes of non-use | after 10 minutes of non-use | after 10 minutes of non-use | after 10 minutes of non-use |
| Dimensions | | 192 x 104 x 52 mm | 192 x 104 x 52 mm | 192 x 104 x 52 mm | 192 x 104 x 52 mm |
| Weight | | 380 g | 380 g | 380 g | 380 g |

Accessories

Mi505-100 Ammonia MR liquid reagent (100 tests)
Mi507-100 Ammonia LR liquid reagent (100 tests)
Mi508-100 Iron HR liquid reagent (100 tests)
Mi512-100 Phosphate LR powder reagent (100 tests)

Mi0001
Mi0002
Mi0003
Mi0005

 Glass cuvettes (2 pcs)
 Caps for cuvettes (2 pcs)
 Stoppers for cuvettes (2 pcs)
 9V battery (1 pc)

Ordering Information

Mi405, Mi407, Mi408 and Mi412 are supplied complete with 2 cuvettes, reagents for 100 tests, hard carrying case, wiping tissue, 9V battery and instructions.

Click to buy: www.easeongear.com

Mi404/Mi406/Mi413/Mi414

Free & Total Chlorine and Chloride Photometers

Milwaukee provides a range of chlorine photometers for all applications: swimming pool treatments, household cleaners, dishwasher additives, laundry powders/liquids and cooling water treatment products all contain chlorine as an oxidizing biocide. Drinking water contains residual chlorine to maintain water purity throughout the supply lines.

Milwaukee offers 3 microprocessor-based instruments with greater resolution, better accuracy and immediate results.

You can choose between three different models:

Mi404 for measuring free (0.00 to 5.00 mg/L) and total (0.00 to 5.00 mg/L) chlorine, **Mi406** for measuring free (0.00 to 5.00 mg/L) chlorine and **Mi413** for measuring free (0.00 to 10.00 mg/L) and total (0.00 to 10.00 mg/L) chlorine.



Chloride is a major constituent of sea water and is extremely corrosive in acidic environments. It requires close monitoring in applications such as marine boiler systems that are effected by seawater contamination.

Chlorides are used by the water treatment professional to determine cycles of concentration in low pressure boilers and cooling systems.

It is essential to monitor chloride concentrations in boiler systems to prevent metal parts being damaged.

In high levels, chloride can corrode stainless steel.



| Specifications | |  Mi404 Free & Total Chlorine |  Mi406 Free Chlorine |  Mi413 Free & Total Chlorine HR |  Mi414 Chloride |
|----------------|---|---|--|--|---|
| Range | Free Chlorine Total Chlorine Chloride | 0.00 to 5.00 mg/L Cl ₂ 0.00 to 5.00 mg/L Cl ₂ | 0.00 to 5.00 mg/L Cl ₂ | 0.00 to 10.00 mg/L Cl ₂ 0.00 to 10.00 mg/L Cl ₂ | 0.00 to 20.00 mg/L Cl ⁻ |
| Resolution | Free Chlorine Total Chlorine Chloride | 0.01 mg/L (0.00 to 3.50 mg/L); 0.10 mg/L (above 3.50 mg/L); 0.01 mg/L (0.00 to 3.50 mg/L); 0.10 mg/L (above 3.50 mg/L) | 0.01 mg/L (0.00 to 3.50 mg/L); 0.10 mg/L (above 3.50 mg/L) | 0.01 mg/L (0.00 to 3.50 mg/L); 0.10 mg/L (above 3.50 mg/L); 0.01 mg/L (0.00 to 3.50 mg/L); 0.10 mg/L (above 3.50 mg/L) | 0.01 mg/L |
| Accuracy | Free Chlorine Total Chlorine Chloride | ±0.04 mg/L @1.50 mg/L ±0.04 mg/L @1.50 mg/L | ±0.04 mg/L @1.50 mg/L | ±0.10 mg/L @5.00 mg/L ±0.10 mg/L @5.00 mg/L | ±0.4 mg/L @10.0 mg/L |
| Method | | adaptation of the USEPA method 330.5 and Standard Method 4500-Cl G | adaptation of the USEPA method 330.5 and Standard Method 4500-Cl G. | adaptation of the USEPA method 330.5 and Standard Method 4500-Cl G. | adaptation of mercury (II) thiocyanate method |
| Light Source | | tungsten lamp | tungsten lamp | tungsten lamp | Blue LED 466 nm |
| Light Detector | | silicon photocell and 525 nm narrow band interference filter | silicon photocell and 525 nm narrow band interference filter | silicon photocell and 525 nm narrow band interference filter | silicon photocell and 466 nm narrow band interference filter |
| Environment | | 0 to 50°C / 32 to 122°F; max RH 100% | 0 to 50°C / 32 to 122°F; max RH 100% | 0 to 50°C / 32 to 122°F; max RH 100% | 0 to 50°C / 32 to 122°F; max RH 100% |
| Battery Type | | 1 x 9V | 1 x 9V | 1 x 9V | 1 x 9V |
| Auto-off | | after 10 minutes of non-use | after 10 minutes of non-use | after 10 minutes of non-use | after 10 minutes of non-use |
| Dimensions | | 192 x 104 x 52 mm | 192 x 104 x 52 mm | 192 x 104 x 52 mm | 192 x 104 x 52 mm |
| Weight | | 380 g | 380 g | 380 g | 380 g |

Accessories

Mi504-100 Free & Total Chlorine liquid reagent set (100 tests)

Mi506-100 Free Chlorine liquid reagent set (100 tests)

Mi513-045 Free & Total Chlorine liquid reagent set (45 tests)

Mi514-100 Chloride liquid reagent set (100 tests)

Mi524-100 Total Chlorine powder reagents (100 tests)

Mi526-100 Free Chlorine powder reagents (100 tests)

Mi0001 Glass cuvettes (2 pcs)

Mi0002 Caps for cuvettes (2 pcs)

Mi0003 Stoppers for cuvettes (2 pcs)



Ordering Information

Mi404, Mi406, Mi413 and Mi414 are supplied complete with 2 cuvettes, reagents, hard carrying case, wiping tissue, 9V battery and instructions.

Click to buy: www.easeongear.com

MW10/MW11**Low cost digital photometers to measure Free & Total Chlorine**

Chlorine is the most commonly used water disinfectant. Applications vary from treatment of drinking water and wastewater to pool and spa sanitization and food processing to sterilization.



Milwaukee offers 2 models:

MW10 for measuring free chlorine (0.00 to 2.50 mg/L) and **MW11** to measure total chlorine (0.00 to 3.50 mg/L).

Key features include:

- User friendly;
- Smaller & Ergonomic case design;
- Inexpensive;
- Larger and Easier to read Display;
- Good accuracy and immediate results;

**Specifications**

| |  MW10 Free Chlorine |  MW11 Total Chlorine |
|--------------------|--|---|
| Range | 0.00 to 2.50 ppm | 0.00 to 3.50 ppm |
| Resolution | 0.01 ppm | 0.01 ppm |
| Accuracy (@ 25 °C) | ±0.03 ppm ±3% of reading | ±0.03 ppm ±3% of reading |
| Typical EMC Dev. | ±0.01 ppm | ±0.01 ppm |
| Light Source | Light Emitting Diode @ 525 nm | Light Emitting Diode @ 525 nm |
| Light Detector | Silicon Photocell | Silicon Photocell |
| Method | Adaptation of USEPA method 330.5. The reaction between free chlorine and the DPD reagent causes a pink tint in the sample. | Adaptation of USEPA method 330.5. The reaction between free chlorine and the DPD reagent causes a pink tint in the sample. |
| Environment | 0 to 50°C (32 to 122 °F) max. 95% RH non-condensing | 0 to 50°C (32 to 122 °F) max. 95% RH non-condensing |
| Battery Type | 1 x 1.5V AAA | 1 x 1.5V AAA |
| Auto-Shut Off | After 2 minutes of non-use | After 2 minutes of non-use |
| Dimensions | 81.5 x 61 x 37.5 mm (3.2 x 2.4 x 1.5") | 81.5 x 61 x 37.5 mm (3.2 x 2.4 x 1.5") |
| Weight | 64 g (2.25 oz.) | 64 g (2.25 oz.) |



They are supplied with 2 cuvettes, 6 reagents, a battery and instruction manual.

**Accessories**

- 2720116** Free Chlorine powder reagent, (25 pcs)
2720216 Total Chlorine powder reagent (25 pcs)



- Mi0011** Glass cuvettes (2 pcs)
Mi0013 Stoppers for cuvetts (2 pcs)
3000300 1.5V AAA batteries (1 pcs)

Ordering information:

All handy photometers are supplied in a carton box including 2 cuvetts, 6 powder reagents, 1 x 1.5 V AAA battery and instructions.

MW12/MW13/MW14




Low cost digital photometers to measure Phosphate, Iron & Iodine

Iron is naturally present in water supplies and therefore needs to be monitored both in potable and industrial applications. Milwaukee offers the **MW14** Iron meter with a range of 0.00 to 5.00 mg/L.

Phosphates are present in natural waters and at concentrations typically found, do not pose any specific health threats to humans. However, excessive contamination of water courses from agricultural fertilizer run off or wastewater/effluent discharge can promote excessive algae or plant growth. Milwaukee offers **MW12** with a range of 0.00 to 2.50 mg/L.

Iodine is used as disinfectant in various applications - one of the most common is the poultry industry waste water treatment. Milwaukee offers **MW13** with a range of 0.0 to 12.5 mg/L.



| Specifications |  MW12 Phosphate |  MW13 Iodine |  MW14 Iron |
|--------------------|--|---|---|
| Range | 0.00 to 2.50 ppm | 0.0 to 12.5 ppm | 0.00 to 5.00 ppm |
| Resolution | 0.01 ppm | 0.1 ppm | 0.01 ppm |
| Accuracy (@ 25 °C) | ±0.04 ppm ±4% of reading | ±0.1 ppm ±5% of reading | ±0.04 ppm ±2% of reading |
| Typical EMC Dev. | ±0.01 ppm | ±0.1 ppm | ±0.01 ppm |
| Light Source | Light Emitting Diode @ 525 nm | Light Emitting Diode @ 525 nm | Light Emitting Diode @ 525 nm |
| Light Detector | Silicon Photocell | Silicon Photocell | Silicon Photocell |
| Method | Adaptation of the Standard Methods for the Examination of Water and Wastewater, 20th edition, Ascorbic Acid method. The reaction between phosphate and the reagent causes a blue tint in the sample. | Adaptation of the Standard Methods for the Examination of Water and Wastewater, 18th edition, DPD method. The reaction between iodine and the reagent causes a pink tint in the sample. | Adaptation of the EPA Phenantroline method 315B, for natural and treated waters. The reaction between iron and reagent causes an orange tint in the sample. |
| Environment | 0 to 50°C (32 to 122 °F) max. 95% RH non-condensing | 0 to 50°C (32 to 122 °F) max. 95% RH non-condensing | 0 to 50°C (32 to 122 °F) max. 95% RH non-condensing |
| Battery Type | 1 x 1.5V AAA | 1 x 1.5V AAA | 1 x 1.5V AAA |
| Auto-Shut Off | After 2 minutes of non-use | After 2 minutes of non-use | After 2 minutes of non-use |
| Dimensions | 81.5 x 61 x 37.5 mm (3.2 x 2.4 x 1.5") | 81.5 x 61 x 37.5 mm (3.2 x 2.4 x 1.5") | 81.5 x 61 x 37.5 mm (3.2 x 2.4 x 1.5") |
| Weight | 64 g (2.25 oz.) | 64 g (2.25 oz.) | 64 g (2.25 oz.) |

Accessories

- 2720115** Phosphate powder reagent, (25 pcs)
2720316 Iodine powder reagent (25 pcs)
2720416 Iron powder reagent, (25 pcs)



- M10011** Glass cuvettes (2 pcs)
M10013 Stoppers for cuvettes (2 pcs)
3000300 1.5V AAA batteries (1 pcs)

Ordering information:

All handy photometers are supplied in a carton box including 2 cuvettes, 6 powder reagents, 1 x 1.5 V AAA battery and instructions.

Click to buy: www.easeongear.com

Mi490 - Photometer
PEROXIDE VALUE in the process of oil making



Mi490 is a user-friendly photometer for monitoring peroxide value in the process of oil making. This instrument will give you direct readings, with a range of 0.0 to 25.0 meq O₂/Kg .

The measurement of the oil's chemical degradation is the peroxide value, which measures the degree to which the oil is oxidized. Rancidification is the decomposition of fats and other lipids by hydrolysis and/or oxidation. Hydrolysis will split fatty acid chains away from the glycerol backbone in glycerides. These free fatty acids can then undergo further auto-oxidation. Oxidation primarily occurs with unsaturated fats by a free radical-mediated process.

One of the most widely used tests for oxidative rancidity, peroxide value is a measure of the concentration of peroxides and hydroperoxides formed in the initial stages of lipid oxidation. Milliequivalents of peroxide per kg of fat are measured by titration with iodide ion.

Peroxide values are not static and care must be taken in handling and testing samples. It is difficult to provide a specific guideline relating peroxide value to rancidity. High peroxide values are a definite indication of a rancid fat, but moderate values may be the result of depletion of peroxides after reaching high concentrations.

Easy Steps


Prepare the sample with oil and the reagent then insert it in the instrument and note the reading.

Accurate Readings

Mi490 will give you direct readings, with a range of 0.0 to 25.0 meq O₂/Kg in the process of oil making.



| Mi490 | Peroxide Value |
|--------------|--|
| Range | 0.0 to 25.0 meq O ₂ /Kg |
| Resolution | 0.5 meq O ₂ /Kg |
| Accuracy | ±0.5 meq O ₂ /Kg |
| Method | adaptation of the CE n. 2568/97 method |
| Environment | 0 to 50°C; max RH 95% |
| Battery Type | 4 x 1.5V AA |
| Auto-off | after 15 minutes of non-use |
| Dimensions | 225 x 85 x 80 mm |
| Weight | 0.5 kg |

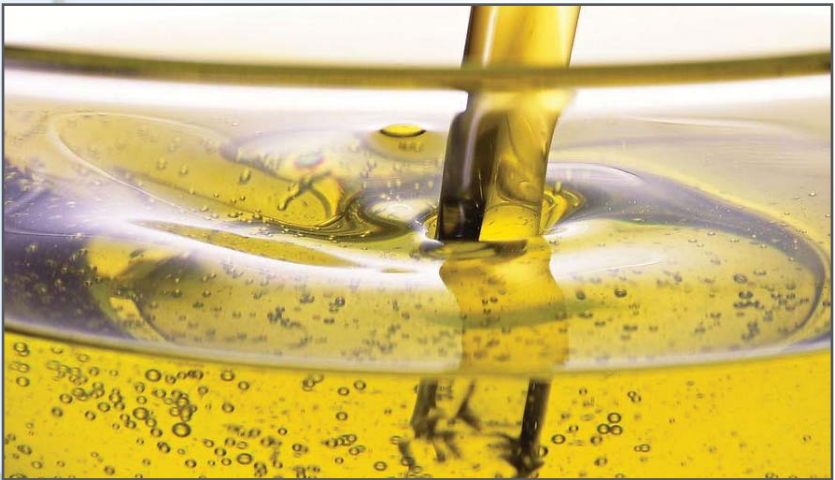

Accessories

- Mi590-021 Peroxides reagent set (21 tests)
- Mi0001 10 mL glass large cuvetts (2 pcs)
- Mi0002 Caps for large cuvetts (2 pcs)
- Mi0004 Tissue for wiping cuvetts (4 pcs)
- Mi0006 Battery 1.5V AA (4 pcs)

Ordering Information

Mi490 is supplied complete with: reagents for 20 tests, 4 x 1 mL syringe, tissue for wiping cuvetts, 4 x 1.5V AA batteries and instruction manual.

Mi415


Turbidity Meter

Turbidity refers to the concentration of undissolved, suspended particles present in a liquid. Turbidity is a measure of the clarity of a sample. For potable water applications turbidity is a good indicator of water quality.

Turbidity Measurement is achieved by analyzing the amount of light refracted from suspended particles such as clay, silt and organic material. By measuring turbidity, by photometric or tube methods, it is possible to estimate suspended solids content.

Mi415 has two operating ranges; 0.00 to 50.00 FNU, and 50 to 1000 FNU that can accommodate the most turbid condition you may encounter.

Mi415 is supplied in a hard carrying case, complete with calibration solutions.



| Specifications | Mi415 Turbidity Meter |
|----------------|--|
| Range | 0.00 to 50.00 FNU; 50 to 1000 FNU |
| Resolution | 0.01 FNU; 1 FNU |
| Accuracy | ±0.5 FNU or ±5% of reading, whichever is greater |
| Method | detection of scattered light |
| Light Source | high emission infrared LED |
| Light Detector | silicon photocell |
| Environment | 0 to 50°C / 32 to 122°F; max RH 100% |
| Battery Type | 1 x 9V |
| Auto-off | after 5 minutes of non-use |
| Dimensions | 192 x 104 x 52 mm |
| Weight | 380 g |



Introduction to Turbidity

The cloudy appearance of water (called Turbidity) is caused by suspended material. The unit of measure adopted by the ISO Standard is the FNU (Formazine Nephelometric Unit) and by EPA is NTU (Nephelometric Turbidity Unit). The other two methods used to test for turbidity and their measurement units are the JTU (Jackson Turbidity Unit) and the Silica unit (mg/L SiO₂). See the conversion table of these methods and their units for your reference.

| | JTU | FTU (NTU/FNU) | SiO ₂ (mg/L) |
|------------------|-------|---------------|-------------------------|
| JTU | 1 | 19 | 2.5 |
| FTU | 0.053 | 1 | 0.13 |
| SiO ₂ | 0.4 | 7.5 | 1 |

Accessories

Mi515-100 AMCO-AEPA-1 @ 0 FNU calibration solution, 30 mL
AMCO-AEPA-1 @ 10 FNU, calibration solution, 30 mL
AMCO-AEPA-1 @ 500 FNU, calibration solution, 30 mL



Mi0011 Glass cuvettes (2 pcs)
Mi0012 Caps for cuvettes (2 pcs)
Mi0013 Stoppers for cuvettes (2 pcs)
Mi0005 9V battery (1 pc)

Ordering Information

Mi415 is supplied complete with 2 cuvettes, calibration solutions, hard carrying case, wiping tissue, 9V battery and instructions.

MA871/MA872/MA873/MA881

Digital Refractometers for Brix, Fructose, Glucose and Invert Sugar Measurements

The digital refractometers are optical instruments that employ the measurement of refractive index to determine the % Brix of sugar (MA871), % Fructose (MA872), % Glucose (MA873) and % Invert Sugar (MA881) in aqueous solutions.





The method is both simple and quick. Samples are measured after a simple user calibration with deionized or distilled water. Within seconds the instruments measure the refractive index of the sample and convert it to % Brix or % by weight concentration units.

The digital refractometers eliminate the uncertainty associated with mechanical refractometers and are easily portable for measurements in the field.

The measurement technique and temperature compensation employ methodology recommended in the ICUMSA Methods Book (Internationally recognized body for Sugar Analysis). Temperature (in °C or °F) is displayed simultaneously with the measurement on the large dual level display along with icons for Low Power and other helpful message codes.

Key features include:

- Dual-level LCD
- Automatic Temperature Compensation (ATC)
- Easy setup and storage
- Battery operation with Low Power indicator (BEPS)
- Automatically turns off after 3 minutes of non-use

| Specifications |  MA871 Brix |  MA872 Fructose |  MA873 Glucose |  MA881 Invert Sugar |
|--------------------------|--|--|--|--|
| Range | 0 to 85% Brix 0 to 80°C / 32 to 176°F | 0 to 85% mass 0 to 80°C / 32 to 176°F | 0 to 85% mass 0 to 80°C / 32 to 176°F | 0 to 85% mass 0 to 80°C / 32 to 176°F |
| Resolution | 0.1% Brix 0.1°C / 0.1°F | 0.1% 0.1°C / 0.1°F | 0.1% 0.1°C / 0.1°F | 0.1% 0.1°C / 0.1°F |
| Accuracy | ±0.2% Brix ±0.3°C / ±0.5°F | ±0.2% ±0.3°C / ±0.5°F | ±0.2% ±0.3°C / ±0.5°F | ±0.2% ±0.3°C / ±0.5°F |
| Light Source | yellow LED | yellow LED | yellow LED | yellow LED |
| Measurement Time | approximately 1.5 seconds | approximately 1.5 seconds | approximately 1.5 seconds | approximately 1.5 seconds |
| Minimum Sample Volume | 100 µL (cover prism totally) | 100 µL (cover prism totally) | 100 µL (cover prism totally) | 100 µL (cover prism totally) |
| Sample Cell | SS ring and flint glass prism | SS ring and flint glass prism | SS ring and flint glass prism | SS ring and flint glass prism |
| Temperature Compensation | automatic between 10 and 40°C / 50 to 104°F | automatic between 10 and 40°C / 50 to 104°F | automatic between 10 and 40°C / 50 to 104°F | automatic between 10 and 40°C / 50 to 104°F |
| Case Material | ABS | ABS | ABS | ABS |
| Enclosure Rating | IP 65 | IP 65 | IP 65 | IP 65 |
| Battery Type | 1 x 9V AA (included) | 1 x 9V AA (included) | 1 x 9V AA (included) | 1 x 9V AA (included) |
| Battery Life | 5000 reading | 5000 reading | 5000 reading | 5000 reading |
| Auto-shut off | after 3 minutes of non-use | after 3 minutes of non-use | after 3 minutes of non-use | after 3 minutes of non-use |
| Dimensions | 192 x 102 x 67 mm | 192 x 102 x 67 mm | 192 x 102 x 67 mm | 192 x 102 x 67 mm |
| Weight | 420 g | 420 g | 420 g | 420 g |

Ordering Information

MA871, MA872, MA873 and MA881 are supplied complete with Mi0005 9V battery and instruction manual.



Stainless Steel Sample
Well and Prism

Place a few drops of the sample in the well and press the READ key.



Click to buy: www.eseasongear.com

MA882/MA883/MA884/MA885

Digital Refractometers for Grape Juice Must Measurements

The **MA882**, **MA883**, **MA884** and **MA885** are optical instruments that are based on the measurement of the refractive index of a solution. The measurement of refractive index is simple and quick and provides the vintner an accepted method for sugar content analysis. Samples are measured after a simple user calibration with deionized or distilled water. Within seconds the instrument measures the refractive index of the grape. This digital refractometers eliminate the uncertainty associated with mechanical refractometers and are easily portable for measurements in the field. The four instruments utilize internationally recognized references for unit conversion and temperature compensation.

- **MA882** measures %Brix;
- **MA883** measures °Baumé;
- **MA884** measures %Brix and Potential Alcohol (% vol);
- **MA885** measures %Brix, °Oechsle (°Oe) and °KMW (°Babo).



Temperature (in °C or °F) is displayed simultaneously with the measurement on the large dual level display along with icons for Low Power and other helpful message codes.

Key features include:

- Dual-level LCD
- Automatic Temperature Compensation (ATC)
- Easy setup and storage
- Battery operation with Low Power indicator (BEPS)
- Automatically turns off after 3 minutes of non-use



Specifications

| |  |  |  |  |
|--------------------------|---|---|---|---|
| | MA882 | MA883 | MA884 | MA885 |
| Range | 0 to 50% Brix 0 to 80°C / 32 to 176°F | 0 to 28 °Baumé 0 to 80°C / 32 to 176°F | 0 to 50% Brix 0 to 25% v/v Potential Alcohol 0 to 80°C / 32 to 176°F | 0 to 50% Brix 0 to 230°Oechsle 0 to 42 °KMW 0 to 80°C / 32 to 176°F |
| Resolution | 0.1% Brix 0.1°C / 0.1 °F | 0.1 °Baumé 0.1°C / 0.1 °F | 0.1% Brix 0.1% v/v Potential Alcohol 0.1°C / 0.1°F | 0.1% Brix 0.1 °Oechsle 0.1 °KMW 0.1°C / 0.1°F |
| Accuracy | ±0.2% Brix ±0.3°C / ±0.5°F | ±0.1 °Baumé ±0.3°C / ±0.5°F | ±0.2% Brix ±0.2 v/v Potential Alcohol ±0.3°C / ±0.5°F | ±0.2% Brix ±1°Oechsle ±0.2 °KMW ±0.3°C / ±0.5°F |
| Light Source | yellow LED | yellow LED | yellow LED | yellow LED |
| Measurement Time | approximately 1.5 seconds | approximately 1.5 seconds | approximately 1.5 seconds | approximately 1.5 seconds |
| Minimum Sample Volume | 100 µL (cover prism totally) | 100 µL (cover prism totally) | 100 µL (cover prism totally) | 100 µL (cover prism totally) |
| Sample Cell | SS ring and flint glass prism | SS ring and flint glass prism | SS ring and flint glass prism | SS ring and flint glass prism |
| Temperature Compensation | automatic between 10 and 40°C / 50 to 104°F | automatic between 10 and 40°C / 50 to 104°F | automatic between 10 and 40°C / 50 to 104°F | automatic between 10 and 40°C / 50 to 104°F |
| Case Material | ABS | ABS | ABS | ABS |
| Enclosure Rating | IP 65 | IP 65 | IP 65 | IP 65 |
| Battery Type | 1 x 9V AA (included) | 1 x 9V AA (included) | 1 x 9V AA (included) | 1 x 9V AA (included) |
| Battery Life | 5000 reading | 5000 reading | 5000 reading | 5000 reading |
| Auto-shut off | after 3 minutes of non-use | after 3 minutes of non-use | after 3 minutes of non-use | after 3 minutes of non-use |
| Dimensions | 192 x 102 x 67 mm | 192 x 102 x 67 mm | 192 x 102 x 67 mm | 192 x 102 x 67 mm |
| Weight | 420 g | 420 g | 420 g | 420 g |

Ordering Information

MA882, **MA883**, **MA884** and **MA885** are supplied complete with Mi0005 9V battery and instruction manual.



Click to buy: www.easeongear.com

MA886

Digital Refractometer for Sodium Chloride Measurements

The **MA886** is an optical instrument that employs the measurement of the refractive index to determine sodium chloride concentration in aqueous solutions used in food preparation.

It is not intended for sea water salinity measurements. The measurement of refractive index is simple and quick and provides the user an accepted method for NaCl analysis. Samples are measured after a simple user calibration with deionized or distilled water. Within seconds the instrument measures the refractive index of the solution.

The digital refractometer eliminates the uncertainty associated with mechanical refractometers and is easily portable for measurements where you need them.

The instrument utilizes internationally recognized references for unit conversion and temperature compensation. It can display the measurement of NaCl concentration 4 different ways: g/100 g, g/100 mL, Specific Gravity, and °Baumé. Temperature (in °C or °F) is displayed simultaneously with the measurement (on 3 of the ranges) on the large dual level display along with icons for Low Power and other helpful message codes.

Key features include:

- Dual-level LCD
- Automatic Temperature Compensation (ATC)
- Easy setup and storage
- Battery operation with Low Power indicator (BEPS)
- Automatically turns off after 3 minutes of non-use



| Specifications | MA886 |
|--------------------------|---|
| Range | 0 to 28 g/100 g 0 to 34 g/100 ml 1.000 to 1.216 Specific Gravity 0 to 26 °Baumé 0 to 80°C / 32 to 176°F |
| Resolution | 0.1 g/100 g 0.1 g/100 ml 0.001 Specific Gravity 0.1 °Baumé 0.1°C / 0.1°F |
| Accuracy | ±0.2 g/100 g ±0.2 g/100 ml ±0.002 Specific Gravity ±0.2 °Baumé ±0.3°C / ±0.5°F |
| Light Source | yellow LED |
| Measurement Time | approximately 1.5 seconds |
| Minimum Sample Volume | 100 µL (cover prism totally) |
| Sample Cell | SS ring and flint glass prism |
| Temperature Compensation | automatic between 10 and 40°C (50 to 104°F) |
| Case Material | ABS |
| Enclosure Rating | IP 65 |
| Battery Type | 1 x 9V AA (included) |
| Battery Life | 5000 reading |
| Auto-shut off | after 3 minutes of non-use |
| Dimensions | 192 x 102 x 67 mm |
| Weight | 420 g |

Ordering Information

MA886 is supplied complete with Mi0005 9V battery and instruction manual.



**Stainless Steel Sample
Well and Prism**

Place a few drops of the sample in the well and press the READ key.

**Liquid Cristal Display
(LCD)**

Dual Level LCD with Primary and Secondary Display.



MA887

Digital Refractometer for Seawater Measurements

The **MA887** is an optical instrument that employs the measurement of the refractive index to determine the salinity of natural and artificial seawater, ocean water or brackish intermediates.

The digital refractometer eliminates the uncertainty associated with mechanical refractometers and is easily portable for ship, shore or home use.

The **MA887** refractometer is an optical device that is simple and quick to use. Samples are measured after a simple user calibration with distilled or deionized water. Within seconds, the refractive index and temperature are measured and converted into one of three popular measurement units; Practical Salinity Units (PSU), Salinity in parts per thousand (ppt), or Specific Gravity (S.G. (20/20)).

All conversion algorithms are based upon respected scientific publications using the physical properties of seawater (not sodium chloride). The temperature (in °C or °F) is also displayed on the large dual level display along with helpful message codes.

Key features include:

- Dual-level LCD
- Automatic Temperature Compensation (ATC)
- Easy setup and storage
- Battery operation with Low Power indicator (BEPS)
- Automatically turns off after 3 minutes of non-use



Years warranty
2

ATC

Dual Display

Self diagnostics

CE

| Specifications | MA887 |
|--------------------------|---|
| Range | 0 to 50 PSU 0 to 150 ppt 1.000 to 1.114 S.G. (20/20) 0 to 80°C / 32 to 176°F |
| Resolution | 1 PSU 1 ppt 0.001 S.G. (20/20) 0.1°C / 0.1°F |
| Accuracy | ±2 PSU ±2 ppt ±0.002 S.G. (20/20) ±0.3°C / ±0.5°F |
| Light Source | yellow LED |
| Measurement Time | approximately 1.5 seconds |
| Minimum Sample Volume | 100 µL (cover prism totally) |
| Sample Cell | SS ring and flint glass prism |
| Temperature Compensation | automatic between 10 and 40°C (50 to 104°F) |
| Case Material | ABS |
| Enclosure Rating | IP 65 |
| Battery Type | 1 x 9V AA (included) |
| Battery Life | 5000 reading |
| Auto-shut off | after 3 minutes of non-use |
| Dimensions | 192 x 102 x 67 mm |
| Weight | 420 g |

Ordering Information

MA887 is supplied complete with Mi0005 9V battery and instruction manual.



Stainless Steel Sample Well and Prism

Place a few drops of the sample in the well and press the READ key.

Liquid Cristal Display (LCD)

Dual Level LCD with Primary and Secondary Display.



Click to buy: www.eseasongear.com

MA888

Digital Refractometer for Ethylene Glycol Measurements

The MA888 is an optical instrument that employs the measurement of the refractive index to determine the % volume and freezing point of ethylene glycol based coolants or antifreeze.

The digital refractometer eliminates the uncertainty associated with mechanical refractometers and is easily portable for use in the field to optimize your cooling system.

The MA888 refractometer is an optical device that is simple and quick to use. Samples are measured after a simple user calibration with distilled or deionized water. Within seconds, the refractive index and temperature are measured and converted into one of two measurement units; % Volume or Freezing Point.

The instrument utilizes internationally recognized references for unit conversion and temperature compensation for ethylene glycol solutions (e.g. CRC Handbook of Chemistry and Physics, 87th Edition).

The temperature (in °C or °F) is also displayed on the large dual level display along with helpful message codes.

Key features include:

- Dual-level LCD
- Automatic Temperature Compensation (ATC)
- Easy setup and storage
- Battery operation with Low Power indicator (BEPS)
- Automatically turns off after 3 minutes of non-use



| Specifications | MA888 |
|--------------------------|--|
| Range | 0 to 100% Volume 0 to -50 °C / 32 to -58 °F Freezing Point 0 to 80°C / 32 to 176°F |
| Resolution | 0.1% Volume 0.1°C / 0.1°F Freezing Point 0.1°C / 0.1°F |
| Accuracy | ±0.2% Volume ±0.5°C / ±1.0°F Freezing Point ±0.3°C / ±0.5°F |
| Light Source | yellow LED |
| Measurement Time | approximately 1.5 seconds |
| Minimum Sample Volume | 100 µL (cover prism totally) |
| Sample Cell | SS ring and flint glass prism |
| Temperature Compensation | automatic between 10 and 40°C (50 to 104°F) |
| Case Material | ABS |
| Enclosure Rating | IP 65 |
| Battery Type | 1 x 9V AA (included) |
| Battery Life | 5000 reading |
| Auto-shut off | after 3 minutes of non-use |
| Dimensions | 192 x 102 x 67 mm |
| Weight | 420 g |

Ordering Information

MA888 is supplied complete with Mi0005 9V battery and instruction manual.



Stainless Steel Sample Well and Prism

Place a few drops of the sample in the well and press the READ key.

Liquid Cristal Display (LCD)

Dual Level LCD with Primary and Secondary Display.



pH600/CD600/CD601/CD610/CD611/CD97




pH/EC & TDS Economical Pocket Testers




Milwaukee's economical testers are easy-to-use and low cost instruments to measure quick and reliable pH, EC or TDS values.

Measuring electrical conductivity is the best way of checking the amount of salt or dissolved solids (TDS) in water. Milwaukee provides you with a range of pocket testers that will allow you to measure from very low to very high conductivity solutions.

All EC/TDS testers compensate for the temperature variance automatically.



| Specifications |  pH600 |  CD600 |  CD601 |
|-----------------------------|--|---|--|
| Range | 0.0 to 14.0 pH | 0 to 1990 ppm | 0 to 1990 μ S/cm |
| Resolution | 0.1 pH | 10 ppm | 10 μ S/cm |
| Accuracy | \pm 0.1 pH | \pm 2% full scale | \pm 2% full scale |
| Calibration | manual, 1 point | manual, 1 point | manual, 1 point |
| Temperature Compensation | | automatic from 5 to 50°C | automatic from 5 to 50°C |
| Environment | 0 to 50°C / 32 to 122°F; max RH 95% | 0 to 50°C / 32 to 122°F; max RH 95% | 0 to 50°C / 32 to 122°F; max RH 95% |
| Battery Type / Battery Life | 3 x 1.5V, alkaline / 700 hours of use | 4 x 1.5V, alkaline / 350 hours of use | 4 x 1.5V, alkaline / 350 hours of use |
| Dimensions / Weight | 150 x 30 x 24 mm / 85 g | 150 x 30 x 24 mm / 85 g | 150 x 30 x 24 mm / 85 g |

| Specifications |  CD610 |  CD611 |  CD97 |
|-----------------------------|--|---|---|
| Range | 0 to 10000 ppm | 0 to 20000 μ S/cm | 0 to 1000 ppm |
| Resolution | 100 ppm | 100 μ S/cm | 1 ppm |
| Accuracy | \pm 2% full scale | \pm 2% full scale | \pm 10 ppm |
| Calibration | manual, 1 point | manual, 1 point | manual, 1 point |
| Temperature Compensation | automatic from 5 to 50°C | automatic from 5 to 50°C | automatic from 5 to 50°C |
| Environment | 0 to 50°C / 32 to 122°F; max RH 95% | 0 to 50°C / 32 to 122°F; max RH 95% | 0 to 50°C / 32 to 122°F; max RH 95% |
| Battery Type / Battery Life | 4 x 1.5V, alkaline / 350 hours of use | 4 x 1.5V, alkaline / 350 hours of use | 4 x 1.5V, alkaline / 350 hours of use |
| Dimensions / Weight | 150 x 30 x 24 mm / 85 g | 150 x 30 x 24 mm / 85 g | 150 x 30 x 24 mm / 85 g |

Accessories

- M10004B pH 4.01 buffer solution 20 mL sachet (25 pcs)
- M10007B pH 7.01 buffer solution 20 mL sachet (25 pcs)
- M10010B pH 10.01 buffer solution, 20 mL sachet (25 pcs)
- M10030B 12880 μ S/cm calibration solution, 20 mL (25 pcs)

- M10031B 1413 μ S/cm calibration solution, 20 mL (25 pcs)
- M10032B 1382 ppm (mg/L) calibration solution, 20 mL (25 pcs)
- M10038B 6.44 ppt (g/L) calibration solution, 20 mL (25 pcs)
- MA9015 Electrode storage solution, 230 mL
- MA9016 Electrode cleaning solution, 230 mL

Ordering Information

pH600, CD600, CD601, CD610, CD611 and CD97 are supplied complete with protective cap, calibration screw-driver, batteries and instructions.

Click to buy: www.eseasongear.com

TH300/TH310

Pocket-sized thermometers
with automatic calibration check

Scientists and laboratory technicians rely on the accuracy of their thermometers when performing routine measurements. For this reason, Milwaukee developed the **TH310**. This palm-sized unit is a highly accurate thermometer that is destined to make glass thermometers obsolete.

Remote temperature measurements require a versatile thermometer with a remote probe that can be used in a hard-to-reach places. The meter must also be easily readable at an angle. The **TH300** is equipped with a stainless steel general purpose probe and 1 meter cable to make remote reading a simple task.

The thermometers have easy-to-read display which shows clear readings at any angle.

| Specifications | TH300 | TH310 |
|-----------------------|--------------------------------|-------------------------------------|
| Range | -50.0 to 150.0°C | -50.0 to 150.0°C |
| Resolution | 0.1°C | 0.1°C |
| Accuracy (@20°C) | ±0.5°C (-20 to 90°C) | ±0.5°C (-20 to 90°C) |
| Typical EMC Deviation | ±0.3°C | ±0.3°C |
| Probe | Stainless steel with 1 m cable | Stainless steel |
| Switch ON/OFF | no | yes |
| Calibration Check | no | yes |
| Environment | 0 to 50°C; max RH 95% | 0 to 50°C; max RH 95% |
| Battery Type | 1 x 1.4V | 1 x 1.5V |
| Battery Life | 1 year approx. | approx 3000 hours of continuous use |
| Dimensions | 106 x 58 x 19 mm | 66 x 50 x 25 mm |
| Weight | 70 g | 50 g |

Ordering Information

TH310 is supplied with stainless steel probe with 1 meter cable, batteries and instruction manual.
TH300 is supplied with batteries and instruction manual.

MT6003
NPK Soil Test Kit

The primary nutrients essential to plant growth and quality are Nitrogen, Phosphorous and Potassium. **N** is associated with plant growth above the ground, **P** is responsible for flower and fruit production as well as overall plant health. **K** promotes disease resistance, water intake and strong root growth.

This kit provides accurate and professional tests and includes 25 sachets of Nitrogen (MT5009), Phosphorous (MT5010) and Potassium (MT5002), 3 x 100 mL bottles of extraction solution and 5 plastic test tubes. All results are compared to standards on laminated colour charts.



Measuring pH in Soil

pH is a measure of the activity of the hydrogen ion (H^+) in the soil solution. If the concentration of H^+ is high, the medium is said to be acid. If it is low, it is said to be alkaline. Most agricultural soils are found between the range 4 to 10 (when measured in water). For practical purposes, soil is neutral when pH is between 6 to 8, depending on plant requirements, and it is acidic when pH is less than 6 and alkaline when it is greater than 8.



1. Collect samples of soil.

Take samples from a homogeneous area per 1000m². In smaller places it is also suggested to take at least two samples (the more samples, the more accurate the measurement will be). Don't take samples from soil where are obvious disorders.

Amount of sample:

Use the same amount of soil for every sample (for example: use identical size sachets)



Spot of sample

General: take the top 5 cm of the ground
Annuals: from 20-40 cm deep
Fruits: from 20-60 cm deep



2. Spread the soil on a paper and let it dry out in a shaded place, or put it into a 40C oven.

3. Shread the dry soil and mix the samples.

You will get a homogeneous sample. It mustn't contain rocks or organic residues. Take a sample from this mixture for the measurement.



4. Sift the soil through a 2mm sifter.

5. Weigh out 1 unit soil (100g is recommended) and put 2 unit (200g, 2dl) destillated water to it.

6. Stir it for 30 seconds. Wait about five minutes.



7. Stir it again then measure the pH of the solution.



Click to buy: www.easeongear.com


Electrodes & Probes pH, ORP, Conductivity, Dissolved Oxygen

CE



Milwaukee has a wide assortment of pH, ORP, Conductivity and other specialty sensors to meet all your specific requirements.

Finding the right electrode for a specific application is a very important task and in order to solve this selection problem it is important to consider the following: electrode body, reference construction and junction. Below you will find a list of Milwaukee electrodes and probes with corresponding instruments they are supplied with.



OTHERS ELECTRODES & PROBES

| | | |
|---|-----------|---|
|  | SE220 | Double junction pH electrode with 1 meter cable and gel filled electrolyte solution (MW100 & MW101 & MW102) |
|  | SE300 | Double junction orp platinum electrode with 1 meter cable and gel filled electrolyte solution (MW500) |
|  | SE510 | Conductivity/TDS probe with 1 meter cable (MW301 & MW401) |
|  | SE520 | Conductivity/TDS probe with 1 meter cable (MW302 & MW402) |
|  | SE600 | Combination probe for pH/EC/TDS with 1 meter cable for MW801 and MW802. |
|  | MA811D/1 | Conductivity/TDS probe with DIN connector and 1 meter cable (for SM301 & SM401) |
|  | MA811/2 | Conductivity/TDS probe with 2 meter cable (for SMS310) |
|  | MA812D/1 | Conductivity/TDS probe with DIN connector and 1 meter cable (for SM302 & SM402) |
|  | MA812/2 | Conductivity/TDS probe with 2 meter cable (for SMS410) |
|  | MA814DB/1 | 4-ring Conductivity/TDS/NaCl/Temperature probe with DIN connector and 1 meter cable (for Mi170 & Mi180) |
|  | MA814D/1 | 4-ring Conductivity/TDS/NaCl/Temperature probe with DIN connector and 1 meter cable (for Mi306) |
|  | MA815/2 | Conductivity probe with 2 meter cable (for SMS315) |
|  | MA816/2 | TDS probe with 2 meter cable (for SMS415) |
|  | MA911B/2 | Double junction, gel filled pH electrode with BNC connector, 2 m cable |
|  | MA921B/2 | Double junction, gel filled ORP electrode with platinum sensor, BNC connector, 2 m cable |
|  | MA831R | Stainless steel Temperature probe with 1 meter cable |
|  | MA840 | Polarographic D.O. probe with 3 meter cable (for SM600 & Mi605) |
|  | MA851D/1 | pH/Conductivity/TDS/Temperature amplified probe with DIN connector and 1 meter cable (for Mi805 & Mi806) |

Click to buy: www.easeongear.com

Electrode Selection Guide

pH, ORP, Conductivity, Dissolved Oxygen

Milwaukee has a wide assortment of pH, ORP, Conductivity and other specialty sensors to meet all your specific requirements.

Before selecting an electrode, please consult the table below. The recommended electrodes are the ones best suited to each application, however we also ask you to verify the specifications on pages 6-7-8-9

Special electrodes for specific applications can also be manufactured upon request.



| Applications | pH | MA905B/3 | MA911B/1 | SE220 | MA913B/3 | MA914BR/1 | MA915B/2 | MA916B/1 | MA916B/3 | MA917B/1 | MA918B/1 | MA919B/1 | MA920B/1 | MA923D/1 | MA991B/1 | ORP | MA921B/1 | SE300 | MA923B/3 | MA924B/1 | Conductivity | SE510 | MA813D/1 | D.O. | MA840 | | |
|---|----|----------|----------|-------|----------|-----------|----------|----------|----------|----------|----------|----------|----------|----------|----------|-----|----------|-------|----------|----------|--------------|-------|----------|------|-------|--|--|
| Agriculture / Soil testing | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Aquarium | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Cheese | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Dairy products | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Emulsions | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Environmental, Pollution | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Fish farming | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Food and beverage (general use) | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Galvanizing waste solution | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Hi purity water | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Heavy duty applications | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| In-line applications | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Laboratory (general use) | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Meat | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Paints | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Paper | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Photographic chemicals | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Strong acid | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Swimming pools | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Water supply | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Wine processing | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Click to buy www.easensgear.com | | | | | | | | | | | | | | | | | | | | | | | | | | | |

Click to buy: www.eseasongear.com

Calibration, Maintenance & Cleaning Solutions

Milwaukee offers a wide range of calibration, maintenance & Cleaning solutions.

The use of calibration and cleaning solutions is fundamental for the correct use of electrodes and for obtaining the most accurate and reproducible readings. Often readings are not correct because the sensors have not been properly handled.

Milwaukee standard solutions are available in 230 mL bottles and 20 mL sachets. Traditional buffer solutions are packed in 230 mL leak-proof bottles and are recommended for lab applications.


Sachets are sealed against light and air and are ideal for on-the-spot calibration.

Simply open, insert the tester or electrode into the sachet and calibrate. Sachets are sold in boxes of 25 pieces.


Calibration, Maintenance & Cleaning Solutions

| | | | |
|--------|--|---------|---|
| MA9001 | pH 1.68 Calibration Buffer Solution, 230 mL | MA9066 | 100% NaCl Calibration Solution, 230 mL |
| MA9004 | pH 4.01 Calibration Buffer Solution, 230 mL | MA9069 | 5000 μ S/cm Conductivity Calibration Solution, 230 mL |
| MA9006 | pH 6.86 Calibration Buffer Solution, 230 mL | MA9070 | Zero Oxygen Solution, 230 mL |
| MA9007 | pH 7.01 Calibration Buffer Solution, 230 mL | MA9071 | Electrolyte Solution for D.O. Probes, 230 mL |
| MA9009 | pH 9.18 Calibration Buffer Solution, 230 mL | MA9112 | pH 12.45 Calibration Buffer Solution, 230 mL |
| MA9010 | pH 10.01 Calibration Buffer Solution, 230 mL | M10000B | Rinse Solution - Deionized Water (box of 25x20 ml sachet) |
| MA9011 | Refilling Electrolyte Solution 3.5M KCl for pH/ORP electrodes, 230 mL | M10004B | pH 4.01 Calibration Buffer Solution (box of 25x20 ml sachet) |
| MA9012 | Refilling Electrolyte Solution 1M KNO ₃ , 230 mL, food applications | M10006B | pH 6.86 Calibration Buffer Solution (box of 25x20 ml sachet) |
| MA9015 | Storage Solution for pH/ORP electrodes, 230 mL | M10007B | pH 7.01 Calibration Buffer Solution (box of 25x20 ml sachet) |
| MA9016 | Cleaning Solution for pH/ORP electrodes, 230 mL | M10009B | pH 9.18 Calibration Buffer Solution (box of 25x20 ml sachet) |
| MA9020 | 200-275 mV ORP Solution, 230 mL | M10010B | pH 10.01 Calibration Buffer Solution (box of 25x20 ml sachet) |
| MA9060 | 12880 μ S/cm Conductivity Calibration Solution, 230 mL | M10016B | Cleaning Solution for electrodes (box of 25x20 ml sachet) |
| MA9061 | 1413 μ S/cm Conductivity Calibration Solution, 230 mL | M10030B | 12880 μ S/cm Calibration Buffer Solution (box of 25x20 ml sachet) |
| MA9062 | 1382 ppm TDS Calibration Solution, 230 mL | M10031B | 1413 μ S/cm Calibration Buffer Solution (box of 25x20 ml sachet) |
| MA9063 | 84 μ S/cm Conductivity Calibration Solution, 230 mL | M10032B | 1332 ppm TDS Calibration Solution (box of 25x20 ml sachet) |
| MA9064 | 80000 μ S/cm Conductivity Calibration Solution, 230 mL | M10038B | 6.44 ppt TDS Calibration Solution (box of 25x20 ml sachet) |
| MA9065 | 111.8 mS/cm Conductivity Calibration Solution, 230 mL | | |

Plastic body pH electrode

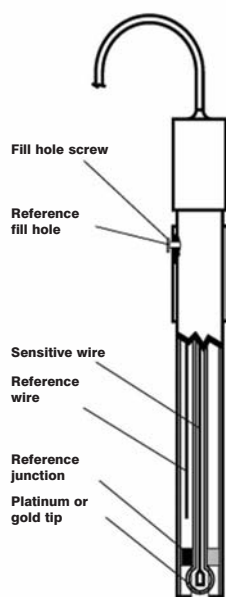

Glass body pH electrode

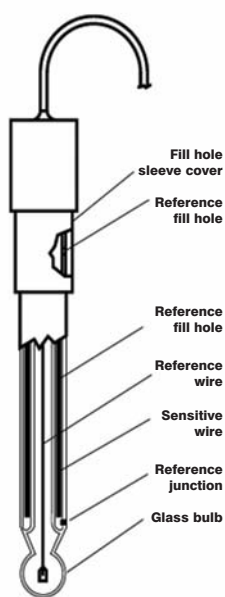

pH Electrode Storage and Maintenance

pH Electrode Storage and Maintenance

To ensure a quick response and free-flowing liquid junction, the sensing element and reference junction must not be allowed to dry out. The following instructions apply to refillable electrodes. For gel-filled electrodes, consult instruction manual.

Routine Storage

Soak electrode in a pH Electrode Storage Solution (MA9015). If a storage solution is unavailable, pH 4 buffer or pH7.01 may be used. The fill hole should be covered to prohibit evaporation of reference fill solution.

Maintenance

Cleaning your electrode between and after use will help extend the life of your electrode and avoid the cost of early replacement.

Routine Cleaning

Soak electrode in MA9016 cleaning solution for half an hour, followed by soaking it in storage solution (MA9015) for at least two hours.

Weekly Maintenance

Inspect electrodes for scratches, cracks, salt crystal buildup, or membrane/junction deposits. Rinse off any salt buildup with distilled water, and remove any membrane/junction deposits as directed in cleaning procedures below. The reference chamber should be drained, flushed with fresh filling solution, and refilled.

WARRANTY POLICY

Milwaukee warrants its instruments to be free of manufacturing defects as follows: bench meters for 3 years, portable and pocket testers for 2 years and electrode/sensors for 6 months (unless otherwise specified).

The warranty period commences from the original date of sale to the user. Warranty is valid only when the product is used under normal conditions and in accordance with the operating limitations and prescribed maintenance procedures.

Milwaukee reserves the right to make improvements in design, construction and appearance of its products without advance notice.

Instrument service

Warranty and non-warranty service are performed by our technicians in Milwaukee headquarters. All items must have a Return Goods Authorization (RGA) number before returning the goods. This number can be obtained by contacting the Milwaukee technical service department at:

tech@milwaukeeinst.com

All products returned without an RGA number will be refused.



FURTHER INFORMATION

Latest updates on new products, technical tips, download of MSDS and free software updates.

Visit our website at:

www.milwaukeeinst.com

for the latest updates on new products, technical tips, download of MSDS, as well as free software updates.

SPECIFIC APPLICATION LITERATURE

Latest updates on new products, technical tips, download of MSDS and free software updates.

Specific application catalogues and leaflets are also available. Please kindly send us an e-mail at:

info@milwaukeeinst.com

Bench Meters



Portable Meters



Click to buy: www.easeongear.com



MARTINI
instruments

Instruments for Water Analysis



pH

ORP

EC

TDS

DO

NaCl

Temp

Brix

NH₃-N

O₂/Kg

FNU

PO₄

Cl₂

Cl⁻

Fe

Measurements made Easy

Authorized Distributor

